


Using MEDIVATORS® ADVANTAGE® Automated Endoscope Reprocessors

Locate the endoscope port and follow the instructions for attaching the corresponding Endoscope Connector. All connectors must be attached.

ADVANTAGE HOOKUP DIAGRAM

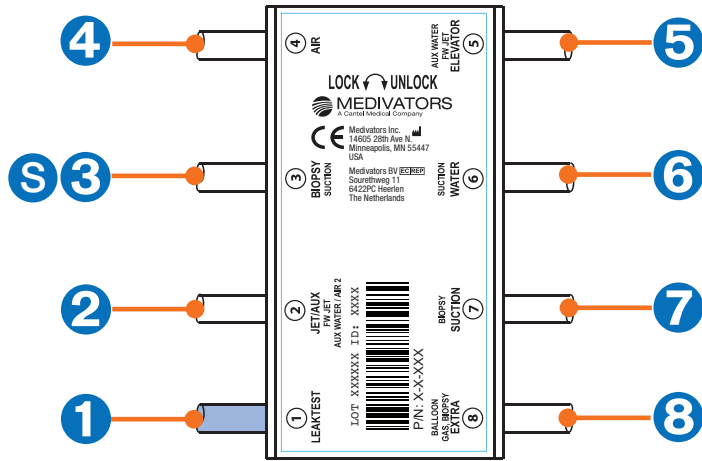

Each ADVANTAGE Hookup is comprised of multiple ports and connector assemblies. Each port is labeled with a Port ID number (circled). This same number also identifies the corresponding Connector Assembly.

CONNECTOR ASSEMBLY IDENTIFICATION CHART

Port ID	Port Name	Connector Assembly Description	Order Number
①	LEAK TEST	Leak Test Connector Assembly	H28715-1
②	JET/AUX	Air/Water Connector Assembly	H28715-26
③	BIOPSY	Biopsy Inlet Connector Assembly	H28715-3
④	AIR	Air Probe Connector Assembly	H28715-4
⑤	ELEVATOR	Auxiliary Water Connector Assembly	H28715-5
⑥	WATER	Air/Water Connector Assembly	H28715-26
⑦	SUCTION	Suction Connector Assembly	H28715-7
⑧	EXTRA	Gas Connector Assembly	H28715-8
①-5	N/A	Air/Water & Suction Port Separator	1-5-111
②	N/A	Gas Cap	75227-521


If a Connector Assembly needs replacement, locate the port number/name and use the corresponding order number found in the chart above. Connector Assemblies are specific to individual hookups.



**Gas Cap**  
Select appropriate cap and insert onto gas port and push to fully engage. The smaller cap fits 10-series endoscopes. The larger cap fits 20-series endoscopes.

**Air/Water & Suction Port Separator**  
Align the separator with the piston ports and push completely home before sliding the frame forward to fully engage.

**Biopsy Inlet Connector**  
Align the biopsy connector disc over the biopsy inlet and push down to compress spring and slide the frame forward to fully engage.

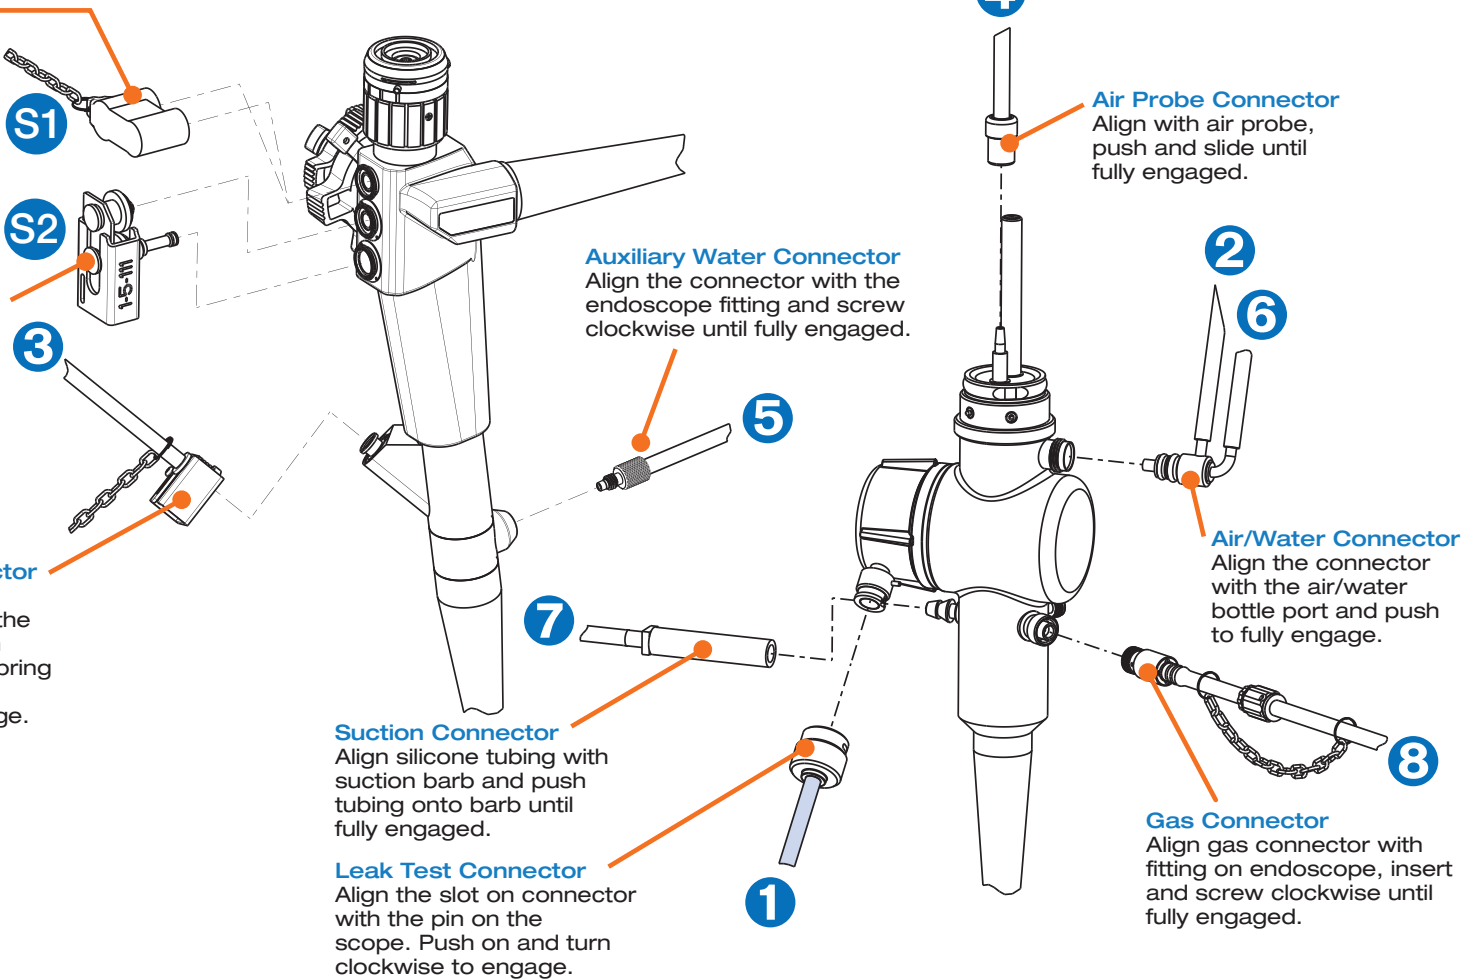

DESIGNATED HOOKUP FOR THE FOLLOWING ENDOSCOPES\*:

CF-100HI	CF-100S	CF-10L	CF-130S	CF-1T10L	CF-1T20L	CF-200I	CF-20L	CF-30I	CF-EL	CF-P20I	CF-V10L	PCF-130L
CF-100HL	CF-100TI	CF-10M	CF-1T100I	CF-1T200I	CF-1TV10L	CF-200L	CF-20M	CF-30L	CF-P10I	CF-P20L	CF-V10S	PCF-20
CF-100I	CF-100TL	CF-130I	CF-1T100L	CF-1T200L	CF-200HI	CF-200S	CF-230I	CF-30M	CF-P10L	CF-P20S	PCF-10	PCF-200
CF-100L	CF-10I	CF-130L	CF-1T10I	CF-1T20I	CF-200HL	CF-20I	CF-230L	CF-EI	CF-P10S	CF-V10I	PCF-130I	PCF-230


\* This list of corresponding endoscope models is subject to change without notice. For a full list, please go to: [www.medivators.com/hookuplookup](http://www.medivators.com/hookuplookup)

Representative endoscope for illustrative purposes only. For exact port locations, refer to endoscope manufacturer's instruction guide.

If you have any questions regarding this hookup, in the U.S., please contact Medivators Technical Support at 1-800-444-4729. Outside the U.S., please contact your Medivators Distributor.

## HOOKUP CONNECTOR BLOCK LABEL

The Hookup Connector Block Label contains useful information for quick reference.

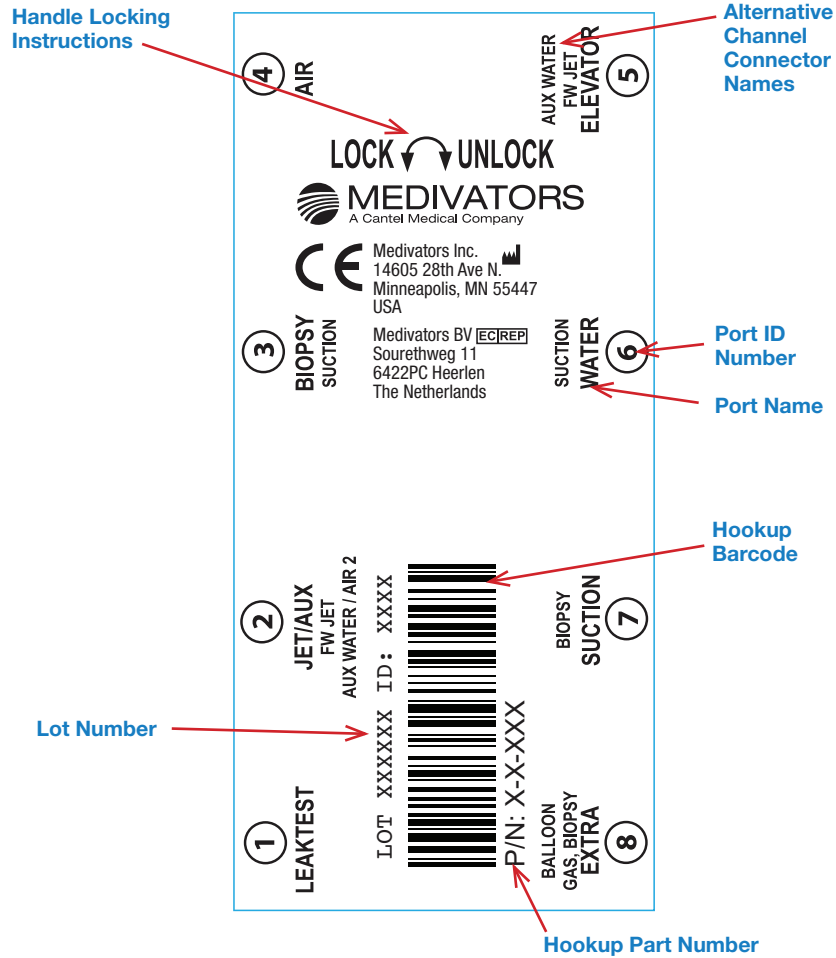

**Handle Locking Instructions** - insert block onto basin channel manifold and move handle to the left to lock. Move to the right to unlock.

**Lot Number** - identifies date of manufacture.

**Hookup Part Number** - identifies hookup.

**Hookup Barcode** - barcode of part number.

**Port Name** - identifier of port location in ADVANTAGE system. Error logs identify issues using these names. Also identifier of Connector Assembly replacements for older model hookups.

**Port ID Number** - identifier for Connector Assembly replacements. Not found on older model hookups.

**Alternative Channel Connector Names** - connector names vary depending on specific endoscope channel configuration.

## WARNINGS & CAUTIONS



This hookup is intended for connection only with the specific endoscope models identified in the appropriate MEDIVATORS online hookup guide. Use of this hookup with endoscopes other than those specified by the hookup application guide may result in inadequate HLD.

Users operating MEDIVATORS AERs and hookups must be trained and competent in the understanding of endoscope channel systems.

Prior to reprocessing, users must verify that the hookup used contains connections for all appropriate channels that require a separate reprocessing connection according to the hookup instructions.

All connectors and adapters must remain firmly attached and unrestricted for the entire disinfection cycle to ensure adequate HLD. Users must inspect the endoscope and hookup combination to verify proper connection and flow.

Modifications or repairs to hookups which do not correspond to the manufacturer's specifications may result in inadequate HLD and/or damage to endoscopes.

Failure to properly clean and prepare endoscope for immersion prior to hookup connection may result in inadequate HLD and/or damage to the endoscope.

Endoscopes must be inspected for damage and verified to be in proper working order prior to hookup connection. Connection of hookups to damaged endoscopes or endoscopes with obstructed/restricted channels could result in inadequate HLD.

Manual leak testing must be carried out in accordance with manufacturer's recommendations prior to reprocessing.

Install all necessary waterproof caps, plugs and cleaning adapters prior to immersion.


Do NOT autoclave MEDIVATORS hookups.

Medivators makes no claim on high-level disinfection efficacy when these reprocessing instructions are not followed, or when this hookup kit is applied to endoscopes other than those specified in the online interactive hookup guide.

Avoid biological contamination. Always wear personal protective equipment when handling endoscopes.



Manufactured in the USA by:

 Medivators Inc.  
14605 28th Avenue North  
Minneapolis, MN 55447 USA  
Toll Free: +1.800.444.4729

 Medivators BV  
Sourethweg 11  
6422PC Heerlen  
The Netherlands  
Tel: +31.45.5.471.471

Cantel Medical Asia/Pacific Pte. Ltd.  
1A International Business Park  
#05-01 Singapore 609933  
Tel: +65.6227.9698

Cantel Medical Devices (China) Co. Ltd.  
Unit 804-805, Innov Tower Block A,  
Hongmei Road, Xuhui 200233 Shanghai  
Tel: +86 21 60161380  
Fax: +86 21 61210913

[www.medivators.com](http://www.medivators.com)